



Decreasing fibrinogen levels are the **first sign of post-partum hemorrhage**, the leading cause of death during childbirth, worldwide



qLabs® FIB

A point-of-care analyser for PPH management to measure Fibrinogen levels within 1 to 10 minutes


Distributed in Australia & New Zealand by:
Diagnostics Stago Pty Ltd
Suite G2, 351 Burwood Hwy, Forest Hill
3131, Victoria, Australia
Ph: 1800 4 78246 email: info@au.stago.com



The lower the level, the faster the time-to-result, helping clinicians to give the right product at the right moment to treat post-partum hemorrhage.




From a single drop of blood, the novel POC device delivers robust, lab comparable results, with integrated hematocrit adjustment



DESIGNED FOR EASE AND SPEED

- No interference from heparin (2 UI/mL) and platelets
- Dry reagent strips stored at room temperature for immediate use
- Individually packed in humidity-resistant pouch
- Lyophilized QC (2 levels)
- Touchscreen handheld rapid testing platform with option of eStation II docking system
- Built-in QR code scanner as well as communications port for printers and computer networks

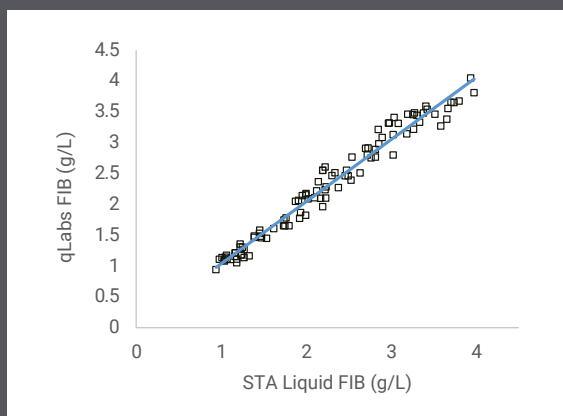

qLabs® FIB test shows very strong correlation with Stago STA®-Liquid Fib test. The correlation coefficient is 0.985 with an intercept of 0.034 and slope of 1.006 (n=98)

FEATURES AND SPECS

Quantification of functional fibrinogen

Clot-based fibrinogen measurement correlated to Clauss fibrinogen method

Sample Type

Venous whole blood in standard coagulation citrated tube (blue cap, 3.2% 0.109 M sodium citrate)

Sample Volume

15 µL

Reportable Range

1.0 – 4.0 g/L (Reference range: 2.0 – 4.0 g/L)

Precision

CV ≤ 7.0%

Hematocrit Range

20% to 60%

Shelf Life at Room Temperature

24 months

Designation	Cat. Nr.	Packaging
qLabs® FIB meter	Q-3 Plus	Unit
eStation II docking station	MBI92	Unit
qLabs® FIB Test strips	QS-18 Pro	24 strips/box
qLabs® FIB Controls level 1	QS-18-CLN	4 x 1 mL
qLabs® FIB Controls level 2	QS-18-CLP	4 x 1 mL